

WHAT IS THE HOMEPUMP ECLIPSE* SYSTEM?

The Homepump* System is a disposable infusion system that delivers your prescribed medication through a catheter (tube). The pump is compact, lightweight and portable.


HOW DOES IT WORK?

The system consists of a balloon type membrane (pump), which holds the medication: The pump provides the pressure to automatically infuse the medication at a preset flow rate. Depending on the size of the pump, infusions will last from 15 minutes to 5 hours. Your nurse will give you detailed instructions about your care.

STORAGE

Your nurse/home health provider will tell you how your medication should be stored.

Make sure the pump is at room temperature during use, or the cold fluid will slow the infusion.

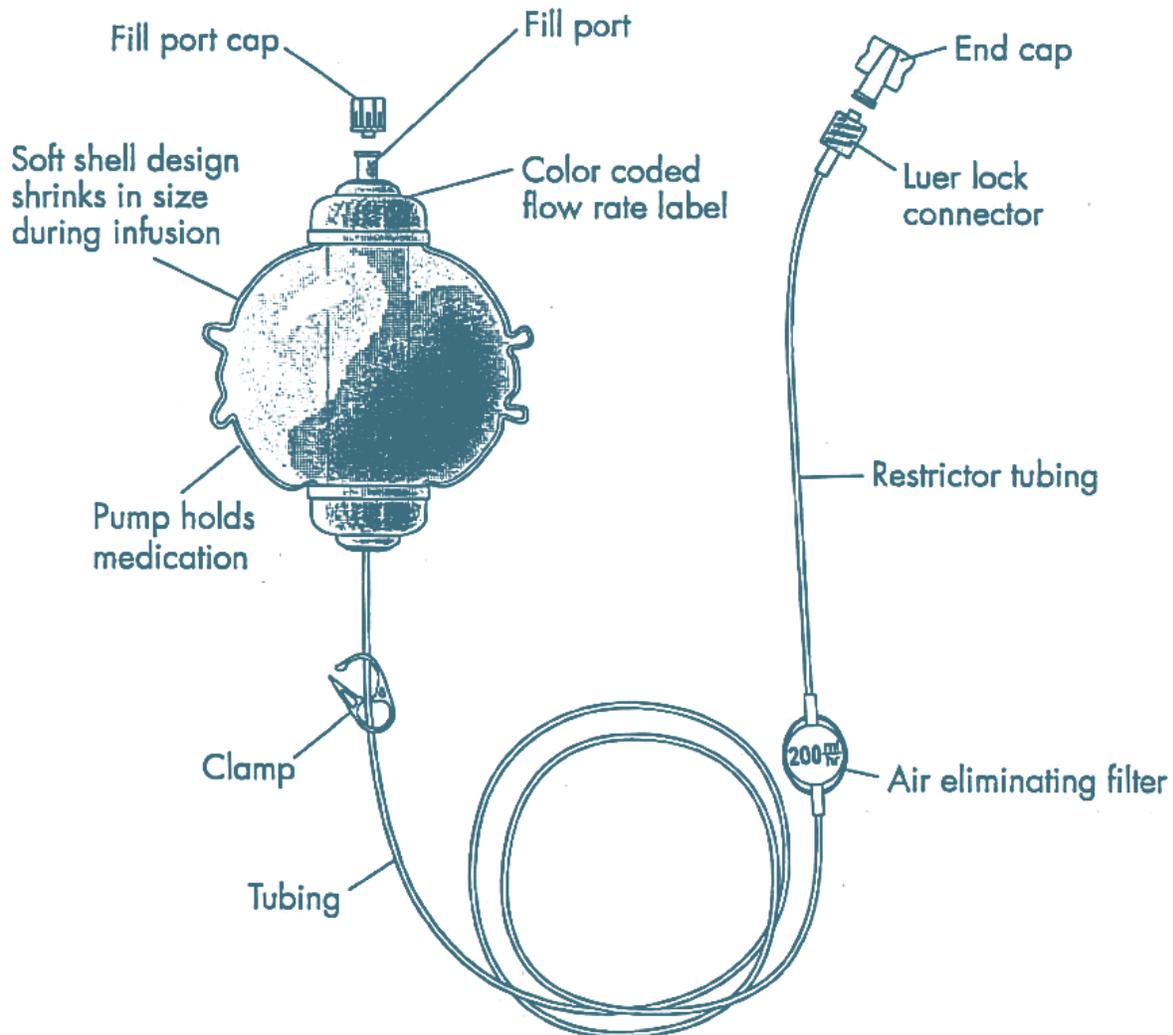

INFUSION

PREPARING THE INFUSION

1. Before Infusing your medication ensure that:

- Your name is correct on the label
- The medication and dose are correct
- Expiration or Use By date has not passed
- The end cap and fill port cap are in place

If any of the above are not correct or missing, DO NOT use the pump. Contact your health care provider.

2. Wash your hands thoroughly with soap and warm water. Dry thoroughly. As instructed by your nurse, follow the procedure on how to clean and prepare your catheter/access device before connecting the pump.

3. You may receive the Homepump * System with the tubing already primed (filled with medication) or you may need to prime the tubing.

Refer to page 2 to see if your pump tubing is primed (filled with medication).

If pump is not primed, follow these steps:

- Remove the end cap on the pump tubing (Figure 1).
- Open the clamp (Figure 2) and wait until you see a drop of medication at the end of the tubing. Allow the tubing to fill with medication.
- When you see the drop at the end of the tubing (Figure 3), close the clamp (Figure 4).




Figure 1




Figure 2



Figure 3




Figure 4

4. Following the connection procedure as instructed by your health care provider, attach the luer lock connector on the pump tubing to your access site.

5. Open the clamp to start the infusion (Figure 2).

INFUSION

DURING THE INFUSION

- Depending on the size of your pump you should notice a change in the look and size of the pump fairly quickly (less than 30 minutes) .
- Do not squeeze the pump. The pump has the force to deliver the medication.

WHEN CARRYING THE PUMP:


- Keep the pump as close as possible to the same level as your catheter/access device.
- During use, place the pump in a carrying case, your pocket, or on a table/bed next to you. Check with your health care provider regarding availability of clips/carrying cases.

SLEEPING: DEPENDING ON YOUR THERAPY, YOU MAY BE USING YOUR PUMP WHILE SLEEPING:

- Make sure the pump is placed on a bedside table or on top of the bed covers.
- Do not place the pump underneath the bed covers where the pump may become too warm.
- Do not place the pump on the floor or hang the pump on a bedpost.

END OF INFUSION

- All your medication has been delivered when the pump is empty.
- The outside bag will be flat and a hard tube can be felt in the middle of the pump.
- Disconnect the pump from your catheter/access device and dispose according to the instructions from your nurse.

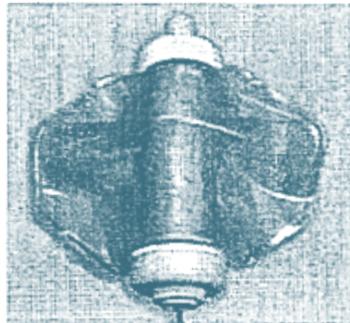

Empty pump



CAUTION: DO NOT REUSE THE PUMP.



TROUBLESHOOTING

If the pump does not seem to be working, make sure:

- The pump is at room temperature.
- The white clamp on the tubing is open (moves freely on the tubing).
- All clamps on your catheter are open.
- There are no kinks in the pump tubing.
- The filter is not taped or covered:
- Follow your nurse's instructions to make sure that your catheter/access device is working.

What to do if the Homepump * System leaks: 1 . Close the clamp on the tubing.

2. If your medication gets on your skin, immediately wash the area with water.
3. Immediately contact your health care provider.
4. Please save the pump for your health care provider to return to the manufacturer.

What to do if the pump tubing becomes disconnected from your catheter/access device:

- DO NOT reconnect.
- Close the tubing clamp and immediately contact your health care provider for instructions.